

Comparison of Sensitivity: Silica Nanoparticles studied by Zetasizer Nano S vs. ZSP coupled online with Centrifugal Field-Flow Fractionation

Dr. Markus J. Spallek, Evelin Moldenhauer
Postnova Analytics GmbH

General Information

ID0026

Technology	CF3-DLS
Info	Postnova CF2000 Centrifugal Field-Flow Fractionation, Malvern Zetasizer Nano S and Nano ZSP
Keywords	Sensitivity Study, Flow-Mode Dynamic Light Scattering, Centrifugal Field-Flow Fractionation

Introduction

Engineered nanoparticles are of widespread use and are nowadays found in various kinds of products in form of additives, thickeners or fillers to obtain products of defined properties for food and cosmetic industry and even for biomedical applications. Investigations regarding environmental issues are also addressed wherein low detection limits as well as high sensitivities are required. The characterization of the nanoparticles is therefore highly important to ensure constant quality as well as reliability. The coupling of Centrifugal FFF with online Dynamic Light Scattering (DLS) by the so called “flow-mode” option is a straight forward technology to combine facile separation and real-time detection of nano- and/or microparticles. The “flow-mode” option is realized by connecting a special quartz flow cell into the detector flow stream delivering accurate size information during the analysis. Besides separation and detection this hyphenated setup allows the user to further enhance the sensitivity and to improve the detection limit bearing the advantage to analyze highly diluted samples. This system features the novel CF2000 coupled directly with a DLS detection device (Malvern Zetasizer Nano Series). The sensitivity levels achieved by either using a Zetasizer Nano S or the novel Zetasizer Nano ZSP are compared. Analysis of a silica (SiO_2) sample mixture showed a 2-times higher sensitivity by choosing the latter device (Nano ZSP).

Comparative Study: Online Sensitivity of Zetasizer Nano Series S and ZSP coupled with CF2000

In the presented application note SiO_2 nanoparticles were used to show the separation efficiency of Centrifugal FFF combined with online-DLS for silica nanoparticles. A 3:2:1 mixture of SiO_2 NPs (w%) with average size diameters of 160 nm, 200 nm and 500 nm diluted in water (MilliQ, 10-18 M Ω) with 0.05% NovaChem100 (v/v) was prepared and injected into the FFF system. In the following the method is briefly addressed: An exponential cross flow proved to be ideal for any kind of nanoparticles to be separated on the Centrifugal FFF. A standard method without further method development was chosen to show the ease of separation on this novel system (advantage of separation by density and hydrodynamic radius). The initial FOCUS step provides enough time for the different sample species to relax (6 min), whereas the ELUTION step gives the start point of sample elution. 10 min of constant centrifugal force (1000 rpm, resp. 20.4% of the maximum rotational speed) is sufficient to ensure nanoparticle separation. An exponential field decay over 80 min was applied. An injection volume of 100 μL was chosen (arbitrarily), but even smaller sample volumes can be injected. Pure water with addition of 0.05% NovaChem100 (v/v) was chosen as eluent.

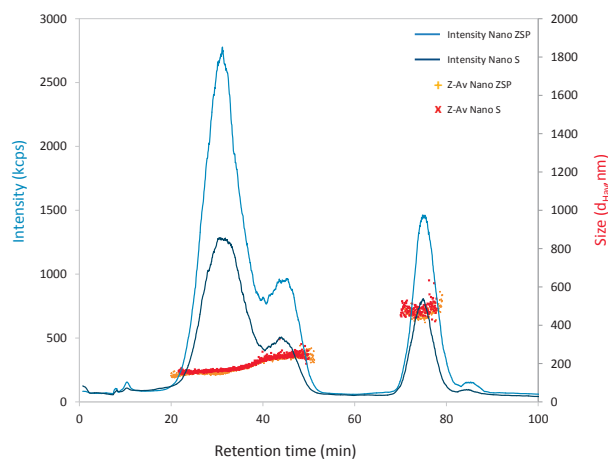


Fig. DLS-fractogram: Silica NP separation using Centrifugal FFF coupled with DLS – Malvern Zetasizer Nano S (dark blue) and ZSP (light blue), red dots hydrodynamic radii.

Conclusion

The hyphenated technology of DLS coupled with Centrifugal FFF proved to be ideal for the investigation of particle sizes (hydrodynamic radius). This was exemplarily shown for the separation of a silica nanoparticle mix in the range of 160 – 500 nm. By choosing the DLS device the sensitivity for detection of these nanoparticles can be further increased. A 2-fold higher sensitivity was obtained by using the Malvern Zetasizer Nano ZSP compared to the Nano S Series. An enhanced optical unit and other technical improvements along with a new laser of higher power (4 mW) renders the Nano ZSP the ideal detector unit for coupling with either Centrifugal FFF (CF2000) or Asymmetrical Flow FFF (AF2000) to obtain hydrodynamic radii information. Whenever a radius of gyration is of interest, a static light scattering device such as the highly sophisticated Multi-Angle Light Scattering (MALS) device PN3621 has to be considered.

References

<http://www.postnova.com/cf2000-overview.html>

<http://www.malvern.com/en/products/product-range/zetasizer-range/zetasizer-nano-range/zetasizer-nano-s/default.aspx>

<http://www.malvern.com/en/products/product-range/zetasizer-range/zetasizer-nano-range/zetasizer-nano-zsp/default.aspx>